


Setting the energy level

The power of the flash has to be set at its maximum in all cases, except for the following skin types:

- Skin type 4: reduce by 1 value
- Skin type 5: reduce by 2 values

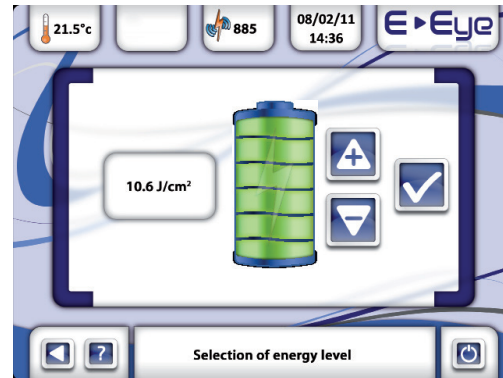

						
	1 White	2 Beige	3 Light Brown	4 Mid Brown	5 Dark Brown	6 Black
Skin type						
	no tan	minimal tan	average tan	deep tan	intense tan	very dark tan
Energy level						

E-EYE

Dry Eye Treatment



IRPL®
INTENSE REGULATED
PULSED LIGHT technology

Your E-EYE specialist:

www.esw-vision.com

ESW vision
part of group E-SWIN

Copyright by ESW vision. All rights reserved. Ref. MM029GB002F08A rev. F 2024/09/05

E-EYE, designed and manufactured by E-SWIN (France), is a class IIb regulated health care device carrying the CE mark (issued by the organization CE 0197). This device is used for the treatment of meibomian blepharitis. Conditions for use described in these instructions must be observed.



E▶EYE

Treatment Protocol

Dry Eye Treatment



Dry Eye Management
One step ahead.

ESW vision

Instructions of use

Before the session:

- Explain the technology and the principle of meibomian gland stimulation to the patient.
- Check for any contraindication to pulsed light.
- Ask the patient to carefully read the informed consent form. ①
- Ask the patient to complete and sign the informed consent form. ②
- Ask the patient to arrive at the session without any cosmetic products on the skin.

At the session:

- Make sure the patient has no contraindications (in particular, no current treatment).
- Make sure there are no cosmetic products on the skin area below the eye (flash zone), and if necessary remove them with a fragrance-free micellar lotion. ③
- Mask any moles and other brown spots within the flash zone with patches.
- Put the safety eye mask on your patient and check the correct positioning. ④
- Apply a generous quantity of gel (minimum 1cm thick) on the lower eyelid (cutaneous flank) and pay attention it does not enter the eye mask. ⑤
- Gradually adjust the power as recommended for setting the energy level and depending on the patient's experience and obtained results. ⑥

- Tap to unlock each safety procedure. 7
- Put on the user **mask** (black). 8
- Apply 5 flashes below each eye 9, starting from the inner canthus of the eye and ending on the temporal region. 10
- Repeat for the other eye. 11
- Switch off the machine at the end of the session.
- Remove the **gel** and rinse the skin. 12

After the session:

- Warn the patient that some redness might appear.
- Tell the patient not to have any other treatment on the flashed areas during the entire cycle of sessions.
- Schedule the second session for two weeks later (Day 15) and then the third session at Day 45 (and an optional fourth session on Day 75).
- Inform the patient to cover the treated zone with sunglasses and use sunscreen on the areas flashed when exposed to UV.

Treatment protocol

The effectiveness of treatment will depend on the application of a specific protocol. This protocol involves 3 sessions administered over the below schedule.

Additional sessions may be scheduled for the consolidation and maintenance of clinical benefits achieved.



